RETURN TO → T60
SH40

KEITHLEY
MODEL 179 DMM
OPERATOR'S MANUAL

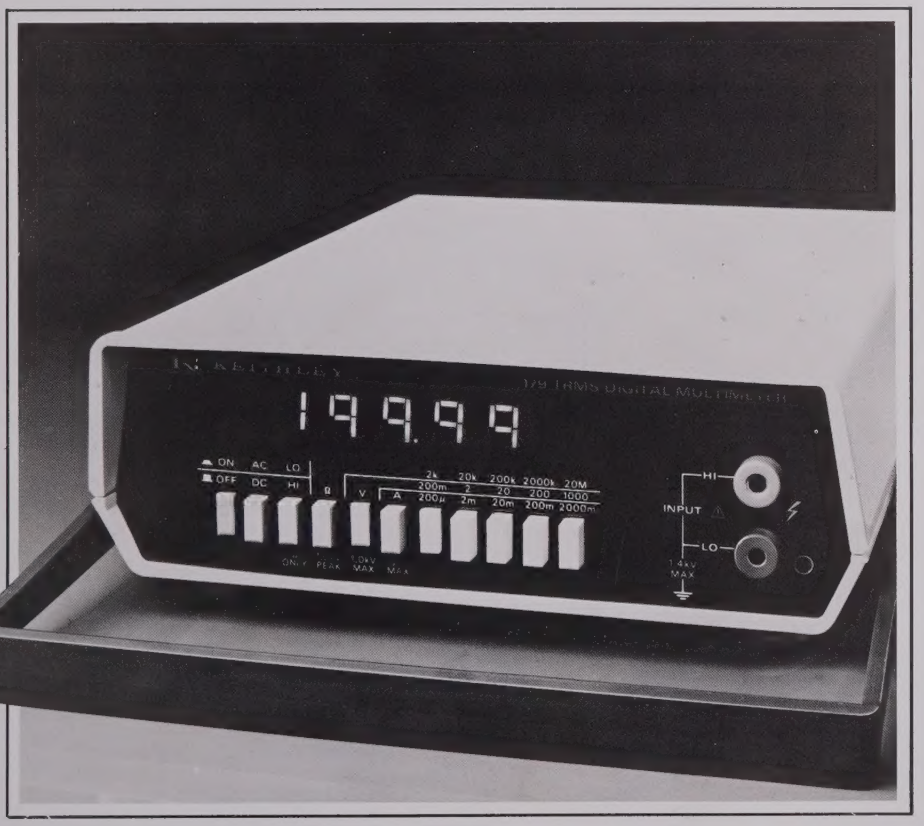

SPECIFICATIONS

DC VOLTAGE

RANGE	MAXIMUM READING	ACCURACY (12 months) 18°–28°C ±(% rdg + digits)	MAXIMUM ALLOWABLE INPUT
200mV	199.99	0.04% + 3d	1200V momentary
2 V	1.9999	0.04% + 1d	1200V momentary
20 V	19.999	0.04% + 1d	1200V
200 V	199.99	0.04% + 1d	1200V
1200 V	1200.0	0.04% + 1d	1200V

Temperature Coefficient (0°–18° and 28°–55°C): ±(0.006% + 0.2 digit)/°C except ±(0.006% + 0.4 digit)/°C on the 200mV range.
Input Resistance: 10MΩ ±0.1%

Normal Mode Rejection Ratio: Greater than 60dB at 50Hz and 60Hz.
Common Mode Rejection Ratio (1kΩ unbalance): Greater than 120dB at DC, 50Hz and 60Hz.
Settling Time: 1 second to within 1 digit of final reading.

AC VOLTAGE

RANGE	MAXIMUM READING	ACCURACY (12 months)* (above 2000 counts) 18°–28°C; 100Hz–10kHz ±(% rdg + digits)	TEMPERATURE COEFFICIENT 0°–18° and 28°–55°C ±(% rdg + digits)/°C 45Hz–10kHz	10kHz–20kHz
200mV	199.99	0.7% + 15d	0.07% + 2d	0.15% + 3d
2 V	1.9999	0.6% + 15d	0.07% + 2d	0.15% + 3d
20 V	19.999	0.5% + 15d	0.05% + 2d	0.05% + 2d
200 V	199.99	0.5% + 15d	0.05% + 2d	0.05% + 2d
1000 V	1000.0	0.5% + 15d	0.05% + 2d	0.05% + 2d

Extended Frequency Accuracy: -(45Hz–100Hz) ±(0.7% + 15 digits) (10kHz–20kHz) ±(0.8% + 15 digits) on the 20V and higher ranges, ±(1.5% + 15 digits) on the 2V range, ±(2% + 15 digits) on the 200mV range.
Response: True root mean square. (AC Coupled)
Crest Factor: 3.

Input Impedance: 1MΩ ±1% shunted by less than 75pF
Maximum Allowable Input Voltage: 1000V rms, 1400V peak, 10^7V•Hz maximum
Common Mode Rejection Ratio (1kΩ unbalance): 60dB at DC, 50Hz and 60Hz.
Settling Time: 2.5 seconds to within 10 digits of final reading.

DC AND AC CURRENT

RANGE	MAXIMUM READING	ACCURACY (12 months)* 18°–28°C +(% rdg + digits) DC	AC 45Hz–10kHz (above 2000 counts)	MAXIMUM VOLTAGE BURDEN	SHUNT RESISTANCE
200μA	199.99	0.2% + 2d	1% + 15d	0.2 V	1kΩ
2mA	1.9999	0.2% + 2d	1% + 15d	0.2 V	100 Ω
20mA	19.999	0.2% + 2d	1% + 15d	0.2 V	10 Ω
200mA	199.99	0.2% + 2d	1% + 15d	0.25V	1 Ω
2000mA	1999.9	0.2% + 2d	1% + 15d	0.6 V	0.1 Ω

Maximum Input: 2A, 250V DC or rms (fuse protected).
Temperature Coefficient (0°–18° and 28°–55°C): DC ±(0.01% + 0.2 digits)/°C. AC ±(0.07% + 2 digits)/°C.
Crest Factor: 3

AC Response: True root mean square. (AC Coupled)
Settling Time: DC: 1 second to within 1 digit of final reading. AC: 2.5 seconds to within 10 digits of final reading.

RESISTANCE

RANGE	MAXIMUM READING	ACCURACY (12 months) 18°–28°C ±(% rdg + digits) HI Ω	LO Ω	MAXIMUM VOLTAGE ACROSS UNKNOWN ON RANGE HI Ω	LO Ω	TEMPERATURE COEFFICIENT 0°–18° and 28°–55°C ±(% rdg + digits)/°C HI Ω	LO Ω	NOMINAL APPLIED CURRENT HI Ω	LO Ω
2kΩ	1.9999	–	0.15% + 15d	–	0.2V	–	0.02% + 2d	–	100μA
20kΩ	19.999	0.04% + 1d	0.15% + 15d	2V	0.2V	0.003% + 0.2d	0.02% + 2d	100μA	10μA
200kΩ	199.99	0.04% + 1d	0.15% + 15d	2V	0.2V	0.003% + 0.2d	0.02% + 2d	10μA	1μA
2000kΩ	1999.9	0.04% + 1d	0.15% + 15d	2V	0.2V	0.003% + 0.2d	0.03% + 2d	1μA	0.1μA
20MΩ	19.999	0.10% + 1d	–	2V	–	0.02 % + 0.2d	–	0.1μA	–

Maximum Allowable Input: 450V rms sustained, 1kV DC or peak AC momentary.
Maximum Open-Circuit Voltage: 5 volts.

Settling Time: 1 second to within 1 digit of final reading except 2 seconds on the 20MΩ range.

GENERAL

DISPLAY: Five 0.5" LED digits, appropriate decimal position and polarity indication.
CONVERSION PERIOD: 400 milliseconds.
ENVIRONMENT:
Operating: 0°C to 55°C; 0% to 80% relative humidity up to 40°C.
Storage: -25°C to +65°C.

POWER: 105–125 or 210–250 volts (switch selected), 90–110V available. 50–60Hz, 7 watts. Optional 6 hour battery pack, Model 1788.
DIMENSIONS, WEIGHT: 85mm high x 235mm wide x 275mm deep (3-1/2 in. x 9-1/4 in. x 10-3/4 in.). Net weight: 1,7kg. (3 lbs., 13 oz).
OVERRANGE INDICATION: Display blinks all zeros above 19999 counts.
MAXIMUM COMMON MODE VOLTAGE: 1400V peak.

*Below 2000 counts, specification is ±(% rdg + 50 digits) typical.

©Copyright 1978, Keithley Instruments, Inc.
Printed in U.S.A.

OPERATING INSTRUCTIONS

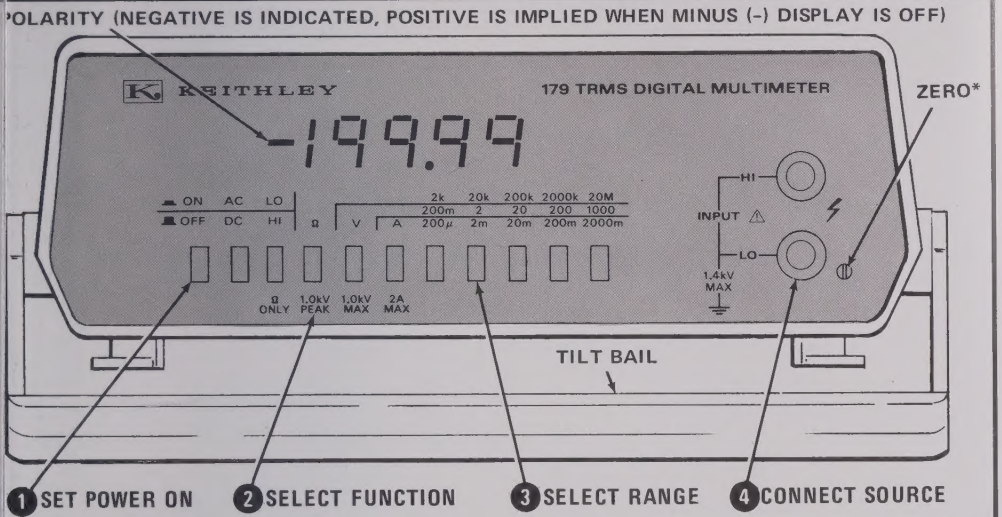

* NOTE: See zero control on second page of Operating Instructions.

(1) **TO OPERATE FROM LINE POWER:**

- Set the Line Switch as described in INITIAL PREPARATION.
- Connect the power cord to line power.
- Set power to **ON.**

TO OPERATE FROM BATTERY POWER:

- Install the Model 1788 as described in INITIAL PREPARATION.
- Charge the Model 1788.
- Disconnect the power cord.
- Set power to **ON.**

(2) **FUNCTION AND RANGE SELECTION:** The pushbuttons are interlocked to avoid improper settings.
(3) The engineering units refer to kilohms (k), megohms (M), millivolts (m), and microamps (μ), or milliamps (m).

DCV: Five ranges are available. The maximum reading is 19999. Overrange is indicated by a flashing 0000 except on the 1200 volt range. Care should be taken not to exceed the maximum ratings. On **DCV**, polarity is displayed automatically and a positive display is implied when the minus display is off.

ACV: Five ranges are available. The maximum reading is 19999. Overrange is indicated by a flashing 0000 except on the 1000 volt range. The Model 179 measures the true root mean square. Crest factor is 3. Frequency response is specified from 45Hz to 20kHz.

Ω(OHMS): Five ranges are available. The maximum reading is 19999. Overrange is indicated by a flashing 0000. Care should be taken not to exceed the maximum ratings.

HI mode includes the 20k, 200k, 2000k, and 20MΩ ranges. Full range voltage drop is 2 volts and is sufficient to cause forward conduction of semiconductor junctions. The **HI** terminal is positive.

LO mode includes the 2k, 20k, 200k, and 2000kΩ ranges. Full range voltage drop is 200mV.

DCA: Five ranges are available. The maximum reading is 19999. Overrange is indicated by a flashing 0000. Overloads are protected by a 2 ampere fuse (installed internally).

ACA: Same as **DCA**. The Model 179 measures the true root mean square. Crest factor is 3. Frequency response is 45Hz to 10kHz.

(4) **INPUT CONNECTIONS:** Use the Model 1681, 1683 or other appropriate banana jack test leads.

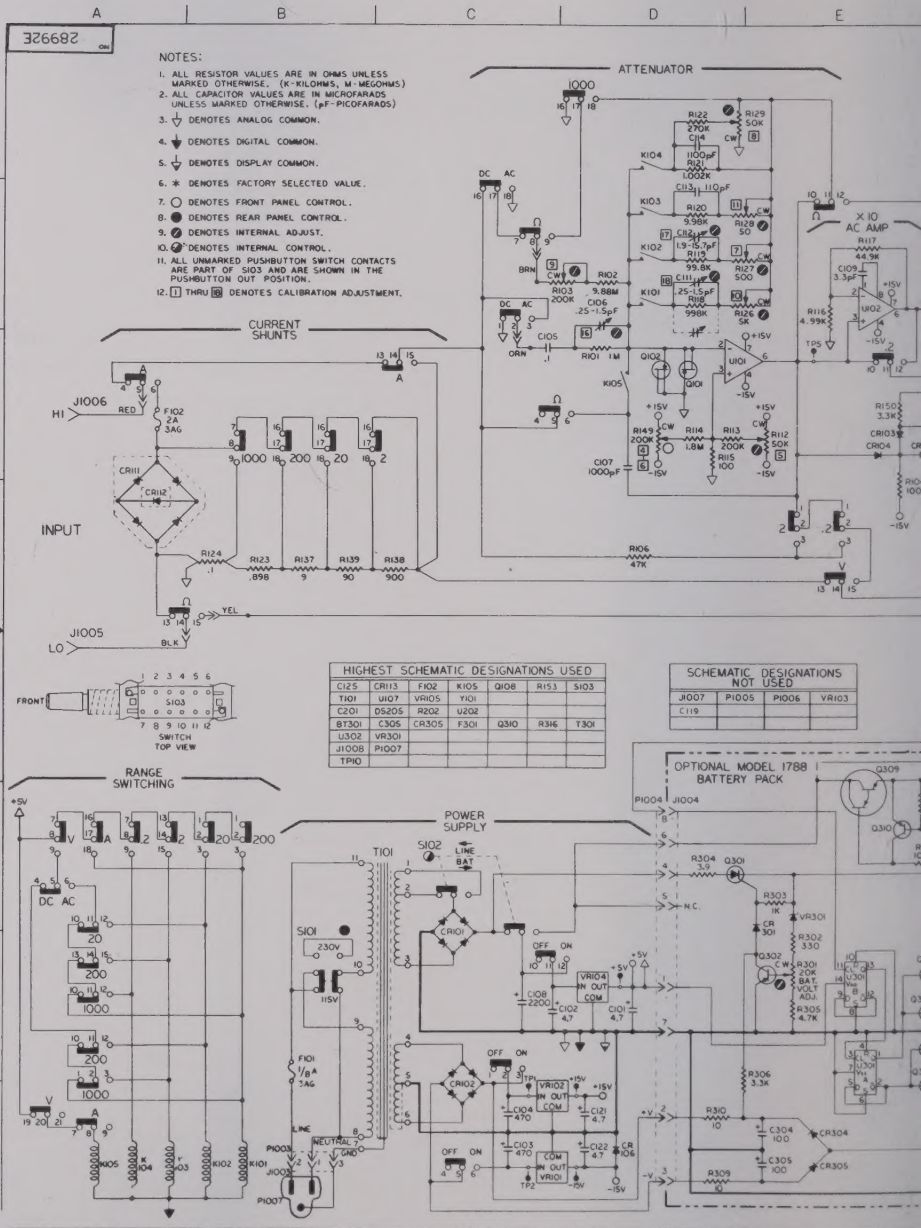
326892
NOTES:
1. ALL RESISTOR VALUES ARE IN OHMS UNLESS MARKED OTHERWISE. (K-KILOHMS, M-MEGOHMS)
2. ALL CAPACITOR VALUES ARE IN MICROFARADS UNLESS MARKED OTHERWISE. (pF-PICOFARADS)
3. DENOTES ANALOG COMMON.
4. DENOTES DIGITAL COMMON.
5. DENOTES DISPLAY COMMON.
6. * DENOTES FACTORY SELECTED VALUE.
7. DENOTES FRONT PANEL CONTROL.
8. DENOTES REAR PANEL CONTROL.
9. DENOTES INTERNAL ADJUST.
10. DENOTES INTERNAL CONTROL.
11. ALL UNMARKED PUSHBUTTON SWITCH CONTACTS ARE PART OF S103 AND ARE SHOWN IN THE PUSHBUTTON OUT POSITION.
12. 1 THRU 16 DENOTES CALIBRATION ADJUSTMENT.
ATTENUATOR
CURRENT SHUNTS
INPUT
J1006
J1005
RANGE SWITCHING
POWER SUPPLY
OPTIONAL MODEL 1788 BATTERY PACK
X10 AC AMP
SWITCH TOP VIEW

HIGHEST SCHEMATIC DESIGNATIONS USED						
C125	CR113	F102	K105	Q108	R153	S103
T101	U107	VR105	Y101			
C201	DS205	R202	U202			
BT301	C305	CR305	F301	Q310	R316	T301
U302	VR301					
J1008	P1007					
TP10						

SCHEMATIC DESIGNATIONS NOT USED			
J1007	P1005	P1006	VR103
C119			

ATIC

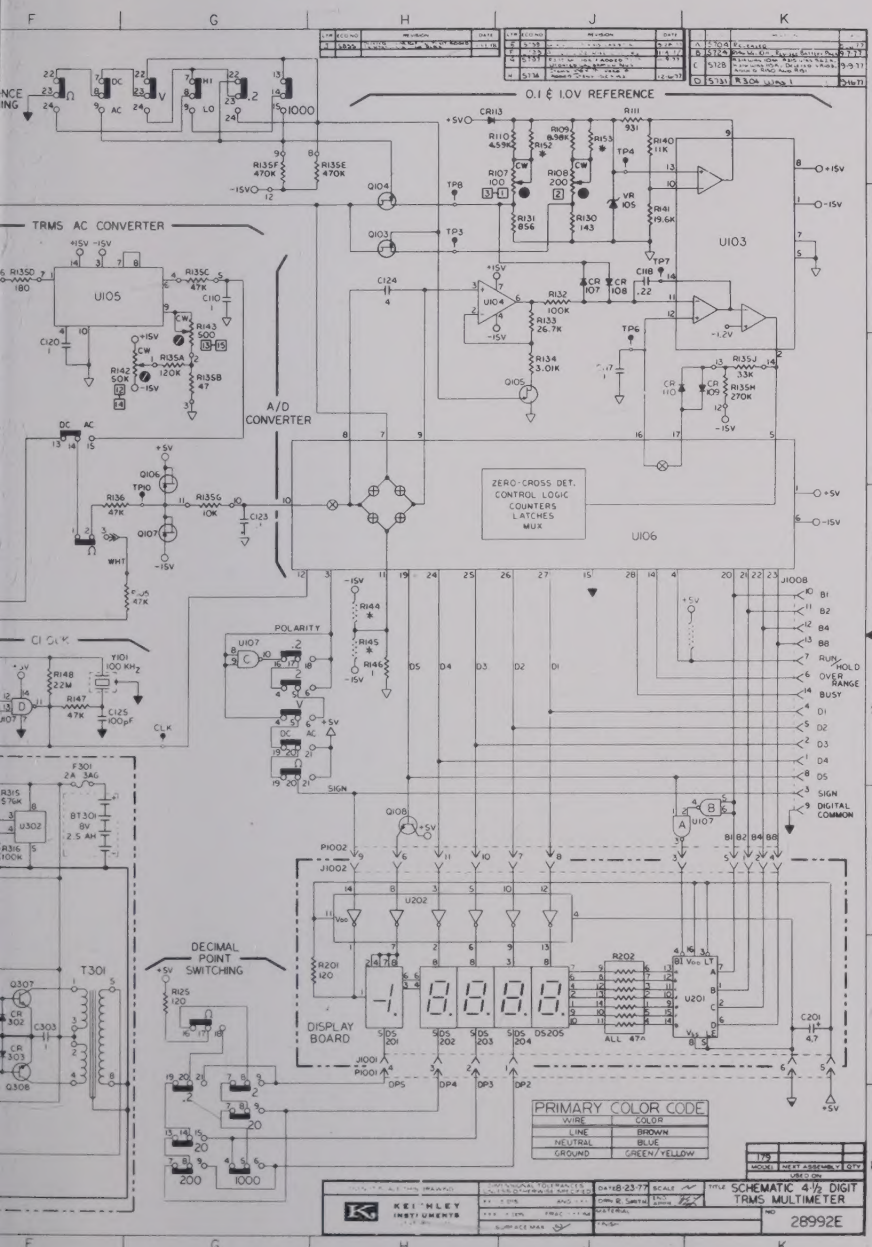
0.1 & 1.0V REFERENCE
TRMS AC CONVERTER
A/D CONVERTER
ZERO-CROSS DET.
CONTROL LOGIC
COUNTERS
LATCHES
MUX
U106
U103
U105
U104
U107
U202
U201
DISPLAY BOARD
DECIMAL POINT SWITCHING
POLARITY
CLOCK
PRIMARY COLOR CODE
WIRE COLOR
LINE BROWN
NEUTRAL BLUE
GROUND GREEN/YELLOW
KEITHLEY INSTRUMENTS
SCHEMATIC 4½ DIGIT TRMS MULTIMETER
28992E

OPERATING INSTRUCTIONS

MAXIMUM RATINGS: ⚠

DCV	(200mV, 2V): 450V rms continuous; 1200V peak, for 8 seconds per minute.
	(20-1200V): 1200V peak.
ACV	(All Ranges): 1000V rms; 1400V peak; 10^7V•Hz.
DCA,ACA	(All Ranges): 2A, 250V DC or rms (fuse protected).
Ω	(All Ranges): 450V rms continuous; 1000V peak, for 8 seconds per minute.

***ZERO CONTROL:** The zero nulls input offset on 20, 200, 1200 **DCV** ranges, and all Ω ranges. Typically, the control may not need adjustment more often than once per week except for environmental conditions outside of the 18°C to 28°C temperature range, or for lead compensation on Ω function. To assure rated accuracy on **DCV** and Ω ranges, set the DMM to **LO** Ω and 200k range, short the input, and adjust **ZERO** for 0000 ±3 digits.

MODEL 1788 RECHARGEABLE BATTERY PACK: The Model 1788 is a field-installed rechargeable battery pack that operates the DMM 6 hours from fully charged batteries. The Model 1788 recharges completely in 14 hours using the built-in charging circuit. Refer to INITIAL PREPARATION for installation instructions.

To charge the Model 1788:
1. Connect the power cord.
2. Set DMM power to **OFF.**
3. Allow the Model 1788 to charge for at least 14 hours.

IMPORTANT

When the DMM is set to power **OFF**, the charge rate is maximum. When the DMM is set to power **ON**, the charge rate is reduced to a trickle charge. For maximum battery life, never leave the Model 1788 in discharged condition.

CALIBRATION AND SERVICING: Calibration and servicing should be performed only by qualified service personnel. Brief calibration instructions are furnished on the internal Calibration Shield. Complete calibration and servicing information is available in the accessory Model 1795 Service Manual.

LINE FUSE RATING: 1/8A, 250V, 3AG, SLOW-BLOW (internally installed)
BATTERY FUSE RATING: 2A, 3AG, FAST-BLOW (installed on Model 1788)
CURRENT FUSE RATING: 2A, 3AG, FAST-BLOW (internally installed)

WARRANTY

We warrant each of our products to be free from defects in material and workmanship. Our obligation under this warranty is to repair or replace any instrument or part thereof, which within a year after shipment, proves defective upon examination. We will pay local domestic surface freight costs.

SERVICE POLICY

For service on your Model 178 or 179 DMM, contact your local representative who will be able to give you immediate assistance in most cases. Complete repair and calibration facilities are maintained in Cleveland, Ohio; Munich, West Germany and Reading, United Kingdom, as well as first line repair service in Palaiseau, France. Information concerning the application, operation or service of your instrument may be directed to the applications engineer at any of the above locations.

Keithley Instruments, Inc., 28775 Aurora Road, Cleveland, Ohio 44139. (216) 248-0400

European Headquarters: Heiglhofstrasse 5, D-8000 Munchen 70 West Germany. (089) 7144065
United Kingdom: 1 Boulton Road, Reading, Berkshire. (0734) 861287
France: 44 Rue Anatole France, F-91121 Palaiseau (01) 928-00-48

INITIAL PREPARATION

SAFETY CONSIDERATIONS

When the DMM is line operated, be sure the "third wire" ground on the power cord is connected to earth ground.

POWER

The DMM can be powered by line voltage or by the optional Model 1788 Rechargeable Battery Pack. Refer to the illustration of the Rear Panel for the following discussion.

(1) Set the Line Switch as shown in the illustration.
CAUTION: Connect only to the line voltage specified. Incorrect line voltage may damage the DMM.

(2) Connect the power cord. The power cord is permanently attached and is conveniently stored by wrapping around the plastic feet and inserting plug end into one of two slots in rear bottom panel.

These adjustments are used only for Calibration. They are not intended for adjustment during operation.

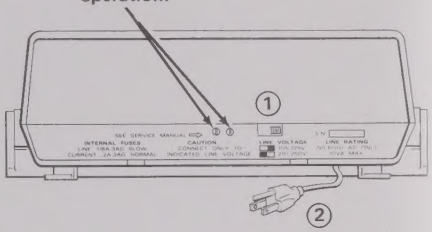

HOW TO REMOVE THE COVER

To gain access to the internal circuit board for installation of the Model 1788 Battery Pack, proceed as follows:

1. Unplug the power cord from line power.
2. Turn the DMM bottom side up.
3. Loosen and remove the slotted screws in 4 holes on the bottom panel.
4. Hold the top and bottom covers together to avoid their separation and turn the DMM over to normal position.
5. Lift off the top cover.
6. To install the top cover again, reverse the procedure.
7. Take care that the four brown plastic spacers that support the Calibration Shield are not disturbed. The spacers are used to support the Model 1788 Battery Pack, when installed, instead of the Calibration Shield.

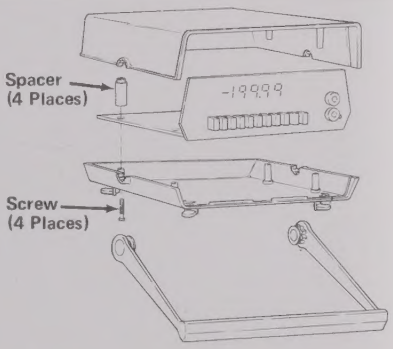

HOW TO INSTALL THE MODEL 1788

1. Disconnect the power cord and set power to **OFF**.
2. Remove the top cover.
3. Lift off the Calibration Shield that is supported by 4 brown plastic spacers. Save the Calibration Shield since it is necessary for proper calibration of the DMM.
4. Set the **BAT/LINE** switch on the DMM circuit board to the **BAT** position. Note that if the switch is not set to **BAT**, the Model 1788 will not function properly.
5. Remove fuse F301 on the Battery Pack.
6. Place the Model 1788 on the brown plastic spacers as shown.
7. Ground clip must make contact with upper side of base of Battery Pack.
8. Plug in the connector from the Model 1788 at location P1004 on the DMM circuit board. Make sure the connector is aligned so that all pins mate properly, otherwise damage to the DMM will result.
9. Install fuse F301 in Battery Pack.
10. Replace the DMM top cover.
11. Reassemble the DMM as described in Cover Removal.
12. Charge the Model 1788.

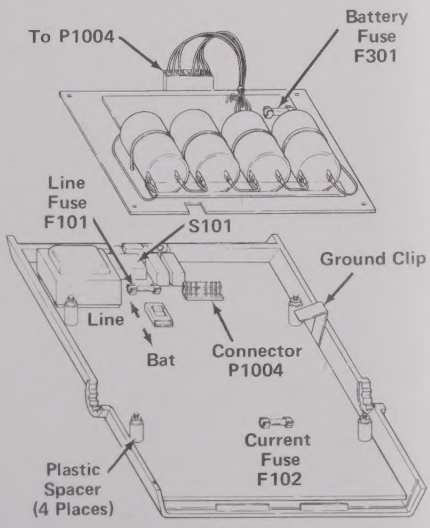

HOW TO CHARGE THE MODEL 1788

1. Connect the power cord
2. Set DMM power to **OFF**.
3. Allow the Model 1788 to charge for at least 14 hours.

IMPORTANT

When the DMM is set to power **OFF**, the charge rate is maximum. When the DMM is set to power **ON**, the charge rate is reduced to a trickle charge. For maximum battery life, never leave the Model 1788 in discharged condition.

ACCESSORIES

Model 1600 High Voltage Probe

The Model 1600 extends the DMM to 40kV. It has a 1000:1 division ratio which means that 1 volt on the DMM corresponds to 1 kilovolt.

To Operate: Set the DMM to **DCV** and appropriate range. Connect the banana plug on the Model 1600 to the **INPUT** terminals. Connect the alligator clip on the Model 1600 to source low. Connect the probe tip to source high.

Specifications:
Voltage Range: 0 to 40,000 volts DC.
Input Resistance: 1000 megohms.
Division Ratio: 1000:1.
Ratio Accuracy
±1.5% at 25kV, decreasing to
±2.0% at 20kV and 30kV
±3.0% at 10kV and 40kV, and
±4.0% at 1kV.
Ratio Stability: ±0.01% per °C; ±0.1% per year.
Heating Effects: Self-heating due to application of high voltage for period in excess of 1 minute will cause a maximum of 0.2% additional error at 40kV (error is less at lower voltage).

Model 1651 50-Ampere Shunt

The Model 1651 allows current measurements to be made up to 50 amperes. It is a 0.001 ohm ±1% 4-terminal shunt. When the DMM is set to the 2 volt range, a fifty ampere current will correspond to 50 millivolts (.0500 volts).



To Operate: Connect separate current leads (not furnished) between the source and the Model 1651 hex-head bolts. Use leads that are rated up to 50 ampere capacity. Connect the voltage leads (furnished) between the Model 1651 screw terminals and the DMM **INPUT** terminals. Set the DMM to **ACV** or **DCV** and 200mV range.

Model 1681 Clip-On Test Lead Set

The Model 1681 contains two leads, 1,2m (48 inches) long, terminated with banana plug and spring-action clip-on probe.



Model 1682 RF Probe

The Model 1682 extends the AC voltage response of the Model 179 from 20kHz to 100MHz.

To Operate: Set the DMM to **DCV** and appropriate range. Connect the Model 1682 to the DMM **INPUT** terminals.

Specifications:
Voltage Range: 0.25 to 30 volts rms.
Transfer Accuracy: ±0.5dB, 100kHz to 100MHz peak responding calibrated in rms of a sinewave.
Input Impedance: 4 megohm shunted by 3pF.
Maximum Allowable Input: 30V rms AC, 200V DC.
Accessories Supplied: straight tip, hook tip, ground clip, hi adapter, banana plug adapter.

Model 1683 Universal Test Lead Kit

Two test leads, 1.2m (48 inches) long with 12 screw-in tips — 2 banana plugs, 2 spade lugs, 2 alligator clips with boots, 2 needle tips with chucks and 4 heavy duty tip plugs.



Model 1684 Carrying Case

The Model 1684 is a hard vinyl case with a fitted foam insert with room for the Service Manual and small accessories.



Model 1685 Clamp-On AC Current Probe

The Model 1685 measures AC current by clamping onto a single conductor. Interruption of the current path is unnecessary. The Model 1685 detects current by sensing magnetic field produced by current.

To Operate: Set the DMM to **ACV** and appropriate range. Connect the Model 1685 to the DMM **INPUT** terminals. The DMM will display 0.1 volts rms per ampere.

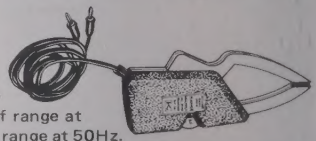

Specifications:
Range: 2, 20 and 200 amperes rms.
Accuracy: ±4% of range at 60Hz. ±6% of range at 50Hz.
Temperature Coefficient: ±0.05%/°C on the 20 and 200 ampere ranges. ±0.3%/°C on the 2 ampere range.
Maximum Allowable Current: 300 amperes rms.
Maximum Conductor Voltage: 600 volts rms.
Conversion Ratio: 0.1 volt rms per ampere.

Model 1010 Single Rack Mounting Kit

The Model 1010 is a single rack mounting kit with overall dimensions 5-1/4 inches (133mm) high and 19 inches (483mm) wide.



Model 1017 Dual Rack Mounting Kit

The Model 1017 is a single/dual mounting kit with overall dimensions 5-1/4 inches (133mm) high and 19 inches (483mm) wide.



Model 1795 Service Manual

The Model 1795 is a complete, illustrated Operating and Service Manual. It includes Theory, Troubleshooting, Calibration, Parts List and Schematic.